For Enjoyable Discovery

CERTIFICATE OF ANALYSIS

Product Name	3X Flag-tag, Cat.#: 318958
Lot No.	MTFB21010-260713
Sequence	MDYKDHDGDYKDHDIDYKDDDDK
Dissolution condition	100%H2O
Modification	N/A
Molecular Weight (MW)	2861.85
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2862.60	Conforms
Purity by HPLC	>95%	95.666%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	500mg	50.0mg*10

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:

Quality Assurance Department

Jul/14/2026

NovoPro Biosciences Inc. VERIFIED Quality Control

Sample Information

Order ID	:MTFB21010
Name	:3X Flag-tag, Cat.#: 318958
Sequence	:MDYKDHDGDYKDHDIDYKDDDDK
Lot. No	:MTFB21010-260713
Pump A	:0.1%Trifluoroacetic in 100% water
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile
Total Flow	:1ml/min
Wavelength	:214nm
Analytial column type	:Kromasil 100-5-C18 (4.6*250mm*5 μm)
Dissolution method	:100%H2O
Inj. Volume	: 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	10
30.00	Pumps	B.Conc	40
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	10
50.00	Controller	Stop	

Chromatogram

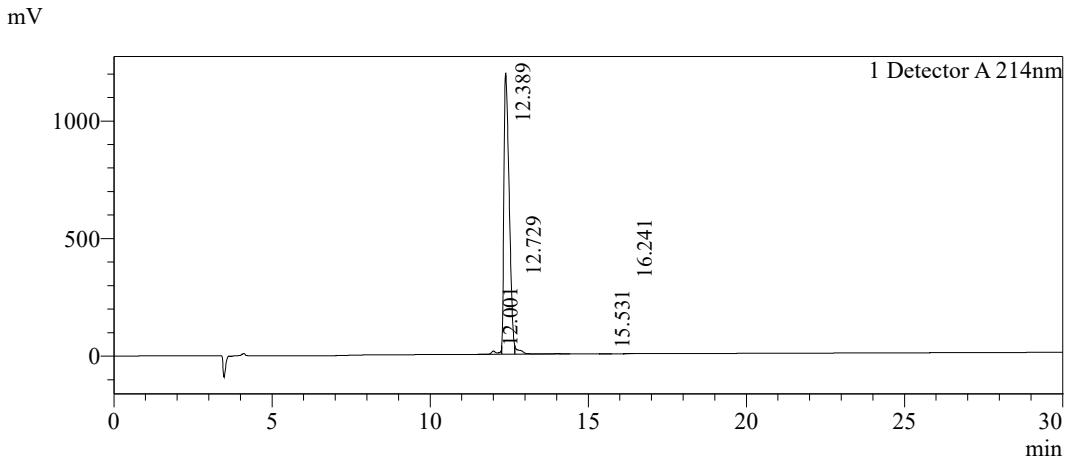

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.001	230894	13855	1.580
2	12.389	13977592	1194013	95.666
3	12.729	396250	21173	2.712
4	15.531	2402	204	0.016
5	16.241	3638	443	0.025
Total		14610776	1229688	100.000

MS Spectrum

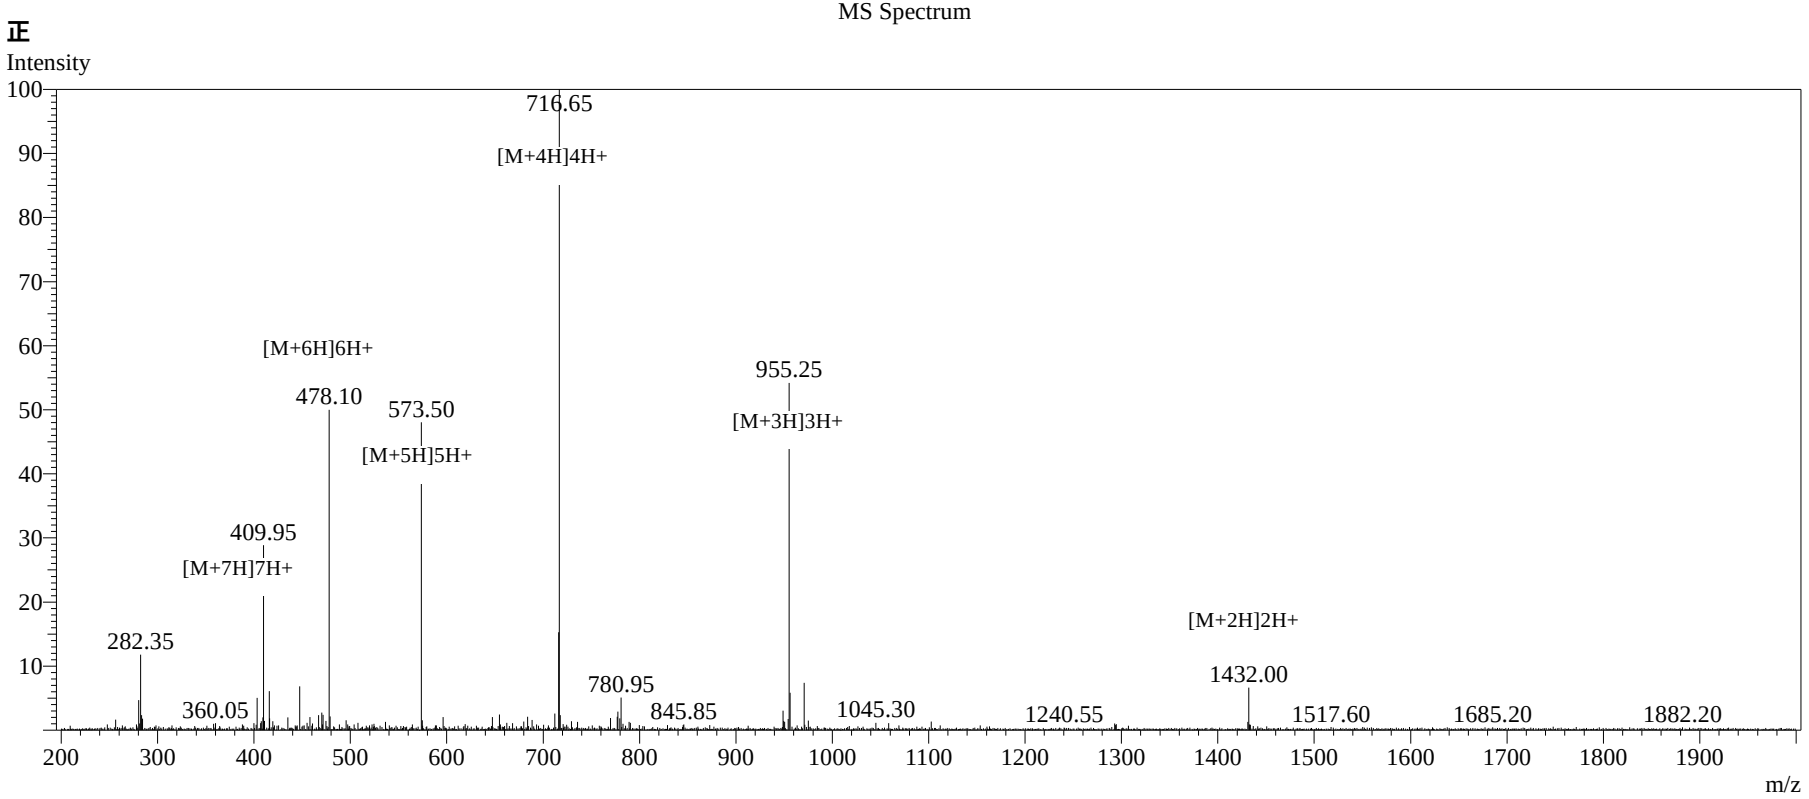

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/07/13 17:26:10	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250℃	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID	:MTFB21010
Name	:3X Flag-tag, Cat.#: 318958
Sequence	:MDYKDHDGDYKDHDIDYKDDDDK
Lot.No	:MTFB21010-260713
Theoretical	:2861.85
Observed	:2862.60