

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	AG-73, Cat.#: 319514 (TFA removed)
<b>Lot No.</b>	MTFA33534-251103
<b>Sequence</b>	RKRLQVQLSIRT (Acetate Salt)
<b>Dissolution condition</b>	100%H <sub>2</sub> O
<b>Modification</b>	acetate salt
<b>Molecular Weight (MW)</b>	1497.79
<b>Storage</b>	-20°C

---

Test Items	Specifications	Results
<b>MW by MS</b>	1498.05	Conforms
<b>Purity by HPLC</b>	>95%	96.758%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	10 mg	5.0mg*2

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Nov/17/2025


Quality Assurance Department



### Sample Information

Order ID	:MTFA33534		
Name	:AG-73		
Sequence	:RKRLQVQLSIRT (Acetate Salt)		
Lot. No	:MTFA33534-251103		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 μm)		
Dissolution method	:100%H2O		
Inj. Volume	: 30ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

### Chromatogram

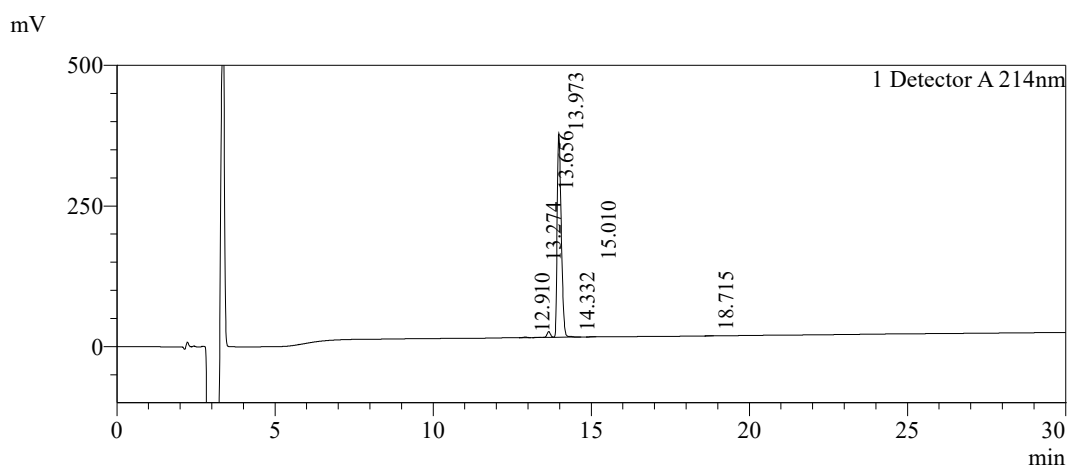


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.910	8816	1115	0.264
2	13.274	1971	261	0.059
3	13.656	78742	10372	2.360
4	13.973	3227986	360800	96.758
5	14.332	12717	1492	0.381
6	15.010	2964	440	0.089
7	18.715	2946	413	0.088
Total		3336142	374893	100.000

# MS Spectrum

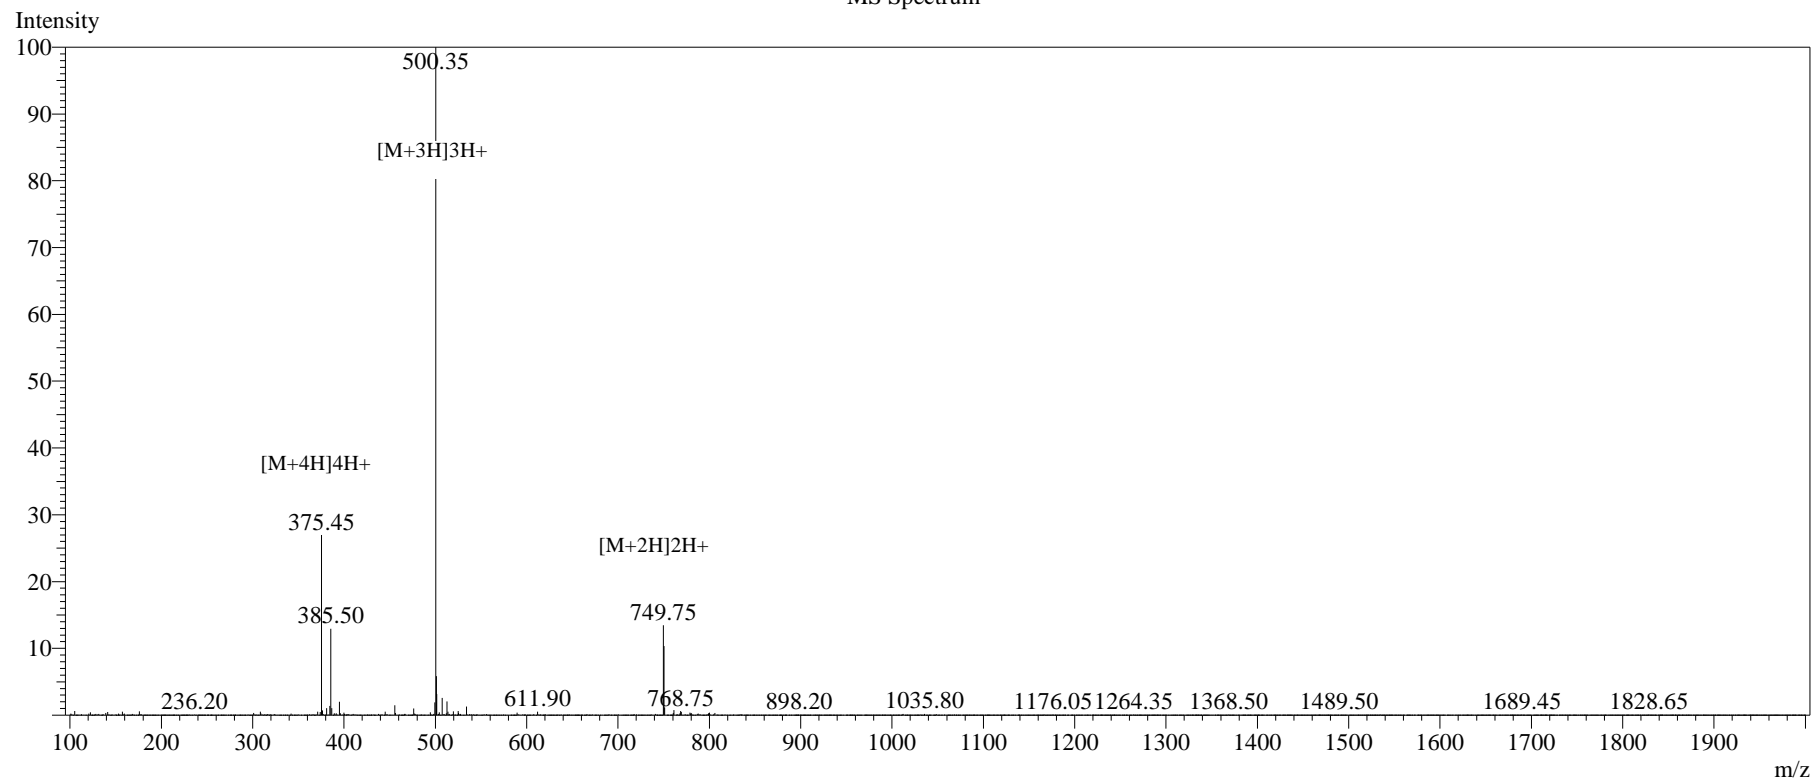

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/11/14 13:24:28	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% ME OH
Order ID	:MTFA33534				
Name	:AG-73				
Sequence	:RKRLQVQLSIRT(Acetate Salt)				
Lot.No	:MTFA33534-251103				
Theoretical	:1497.79				
Observed	:1498.05				