

CERTIFICATE OF ANALYSIS

Product Name	EPO mimetic peptide-1, Cat.#: 319826 (TFA removed)
Lot No.	P260708-CL674476
Sequence	H-GGTYSCHFGPLTWVCKPQGG-NH ₂ (Disulfide bond: Cys6-Cys15)
Dissolution condition	100%H ₂ O
Modification	Acetate salt
Molecular Weight (MW)	2092.20
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2092.36	Conforms
Purity by HPLC	>95%	97.87%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Peptide content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Jul/30/2026


Quality Assurance Department



Sample Information

Order ID : 71929
 Name : EPO mimetic peptide-1, Cat.#: 319826 (TFA removed)
 Sequence : H-GGTYSCHFGPLTWVCKPQGG-NH2
 (Disulfide bond: Cys6-Cys15)
 Lot. No : P260708-CL674476
 Pump A : 0.1% Trifluoroacetic in 100% Acetonitrile
 Pump B : 0.1% Trifluoroacetic in 100% Water
 Total Flow : 1ml/min
 Wavelength : 220nm
 Analytical column type : 4.6*250mm C18
 Dissolution method : 100% H₂O

Chromatogram

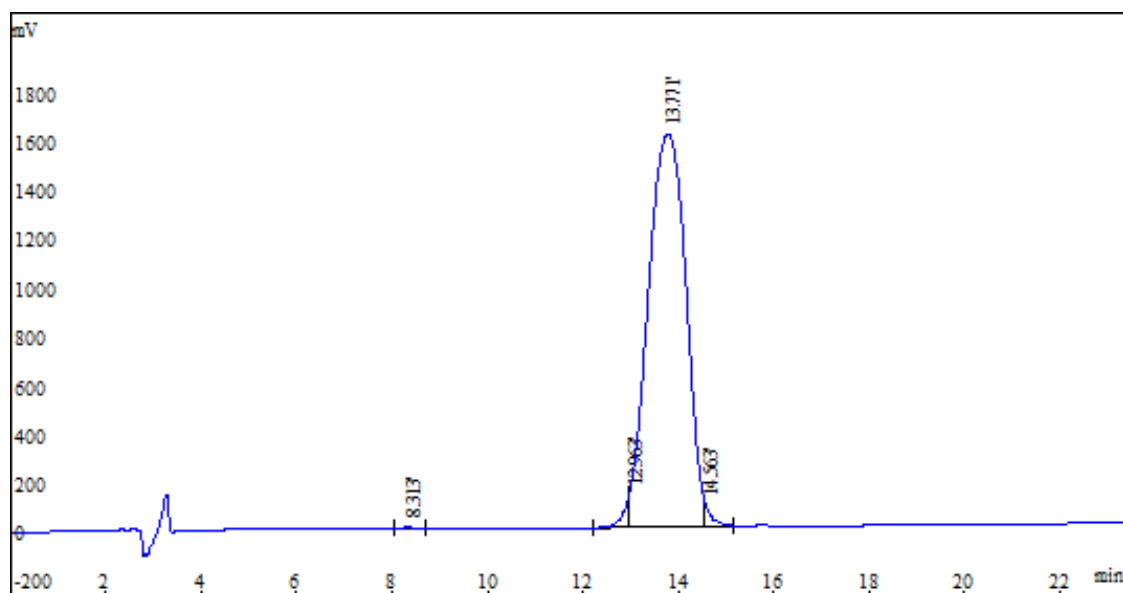


Peak Table

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.313	130751	9010	0.1466
2	12.963	1075615	133562	1.206
3	13.771	87265715	1602543	97.87
4	14.563	692424	82706	0.7766
Total	-	89164505	1827821	100

MS Spectrum

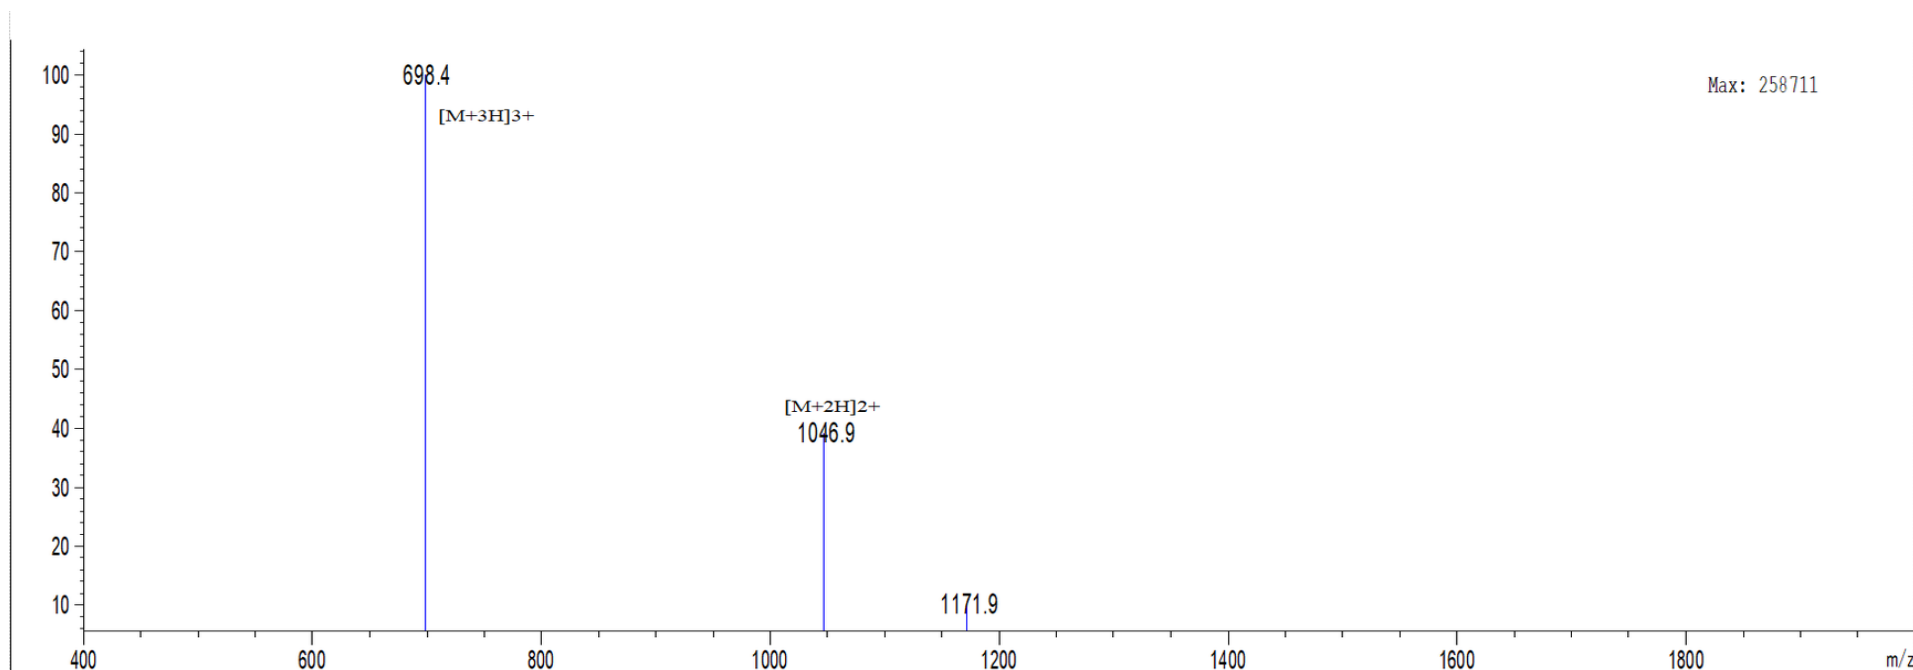

Sample Information

Date Acquired	: 2026/07/20	Interface	: ESI	Prerod Bias	: +4.5kv
Block Temp	: 200°C	Nebulizing Gas Flow	: 1.5L/min	Detector	: 1.5kv
Injection Volume	: 1ul	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
		CDL Volt	: -20.0v	B.conc	: 50%H2O/50%ACN
Order ID	: 71929				
Name	: EPO mimetic peptide-1, Cat.#: 319826 (TFA removed)				
Sequence	: H-GGTYSCHFGPLTWVCKPQGG-NH2 (Disulfide bond: Cys6-Cys15)				
Lot.No	: P260708-CL674476				
Theoretical	: 2092.36				
Observed	: 2092.20				