

---

**CERTIFICATE OF ANALYSIS**


<b>Product Name</b>	HGH Fragment 176-191 peptide, Cat.#: 318938 (TFA removed)
<b>Lot No.</b>	MTFB20708-260407
<b>Sequence</b>	YLRIVQC*RSVEGSC*GF (Acetate Salt)
<b>Dissolution condition</b>	15%ACN+85%H2O
<b>Modification</b>	disulfide bridge, acetate salt
<b>Molecular Weight (MW)</b>	1815.09
<b>Storage</b>	-20°C

---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
MW by MS	1815.40	Conforms
Purity by HPLC	>95%	98.794%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	80mg	5.0mg*16

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:   
Quality Assurance Department

Apr/14/2026




### Sample Information

Order ID :MTFB20708  
 Name :HGH Fragment 176-191 peptide, Cat.#: 318938 (TFA removed)  
 Sequence :YLRIVQC\*RSVEGSC\*GF (Acetate Salt)  
 Lot. No :MTFB20708-260407  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Kromasil 100-5-C18 (4.6\*250mm\*5 µm)  
 Dissolution method :15%ACN+85%H2O  
 Inj. Volume : 50ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

### Chromatogram

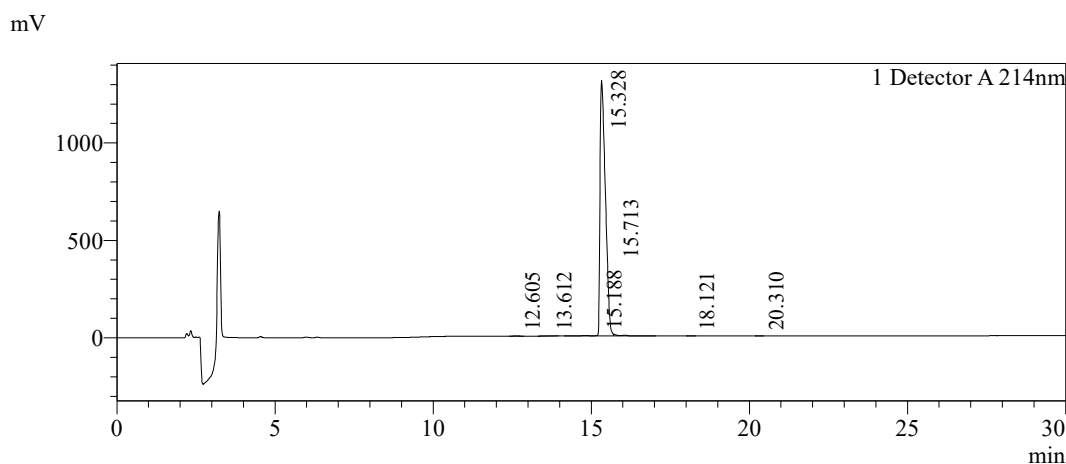


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.605	4150	287	0.026
2	13.612	6794	428	0.043
3	15.188	53349	2331	0.340
4	15.328	15487637	1311231	98.794
5	15.713	120447	9528	0.768
6	18.121	1646	252	0.011
7	20.310	2741	416	0.017
Total		15676764	1324473	100.000

### MS Spectrum

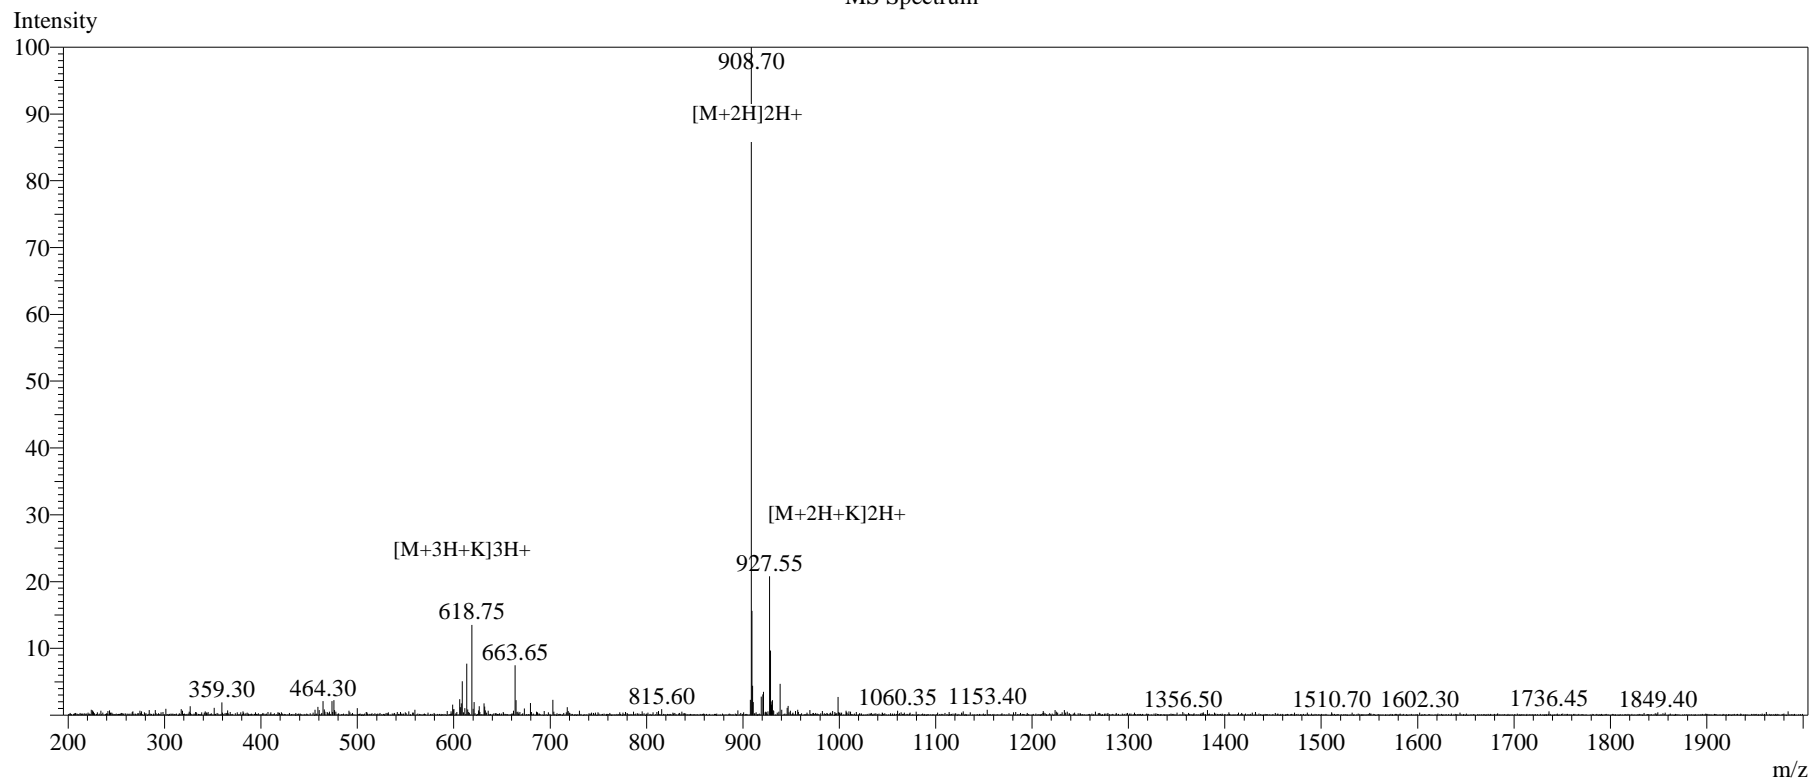

### Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/04/10 10:53:33	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:MTFB20708
Name	:HGH Fragment 176-191 peptide, Cat.#: 318938 (TFA removed)
Sequence	:YLRIVQC*RSVEGSC*GF (Acetate Salt)
Lot.No	:MTFB20708-260407
Theoretical	:1815.09
Observed	:1815.40