

CERTIFICATE OF ANALYSIS

Product Name	LANA peptide, Cat.#: 319154
Lot No.	MTFA32941-250613
Sequence	MAPPGMRLRSGRSTGAPLTRGSC
Dissolution condition	100%H ₂ O
Length	AA
Modification	N/A
Molecular Weight (MW)	2359.73
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2359.80	Conforms
Purity by HPLC	>95%	95.773%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	30mg	5.0mg*6

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Jun/18/2025

Quality Assurance Department




Sample Information

Order ID	:MTFA32941		
Name	:LANA peptide		
Sequence	:MAPPGMRLRSGRSTGAPLTRGSC		
Lot. No	:MTFA32941-250613		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H ₂ O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

mV

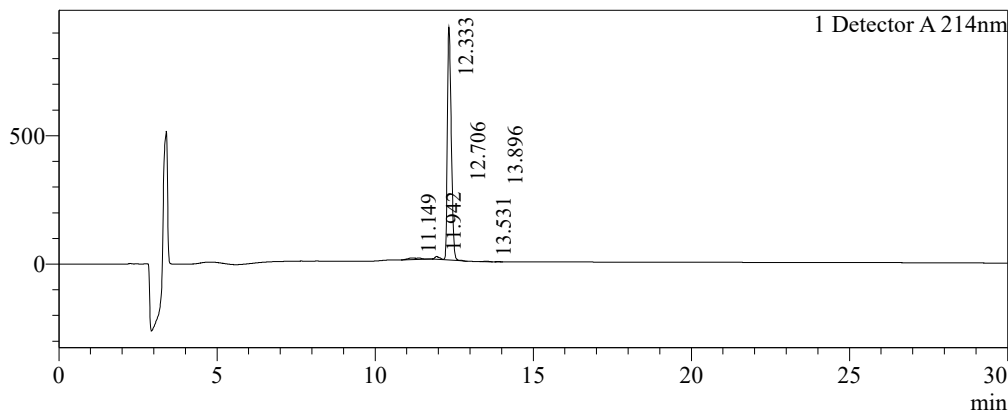


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	11.149	182843	6560	2.245
2	11.942	125082	11704	1.536
3	12.333	7799543	906577	95.773
4	12.706	14488	2398	0.178
5	13.531	18296	2099	0.225
6	13.896	3528	501	0.043
Total		8143780	929840	100.000

MS Spectrum

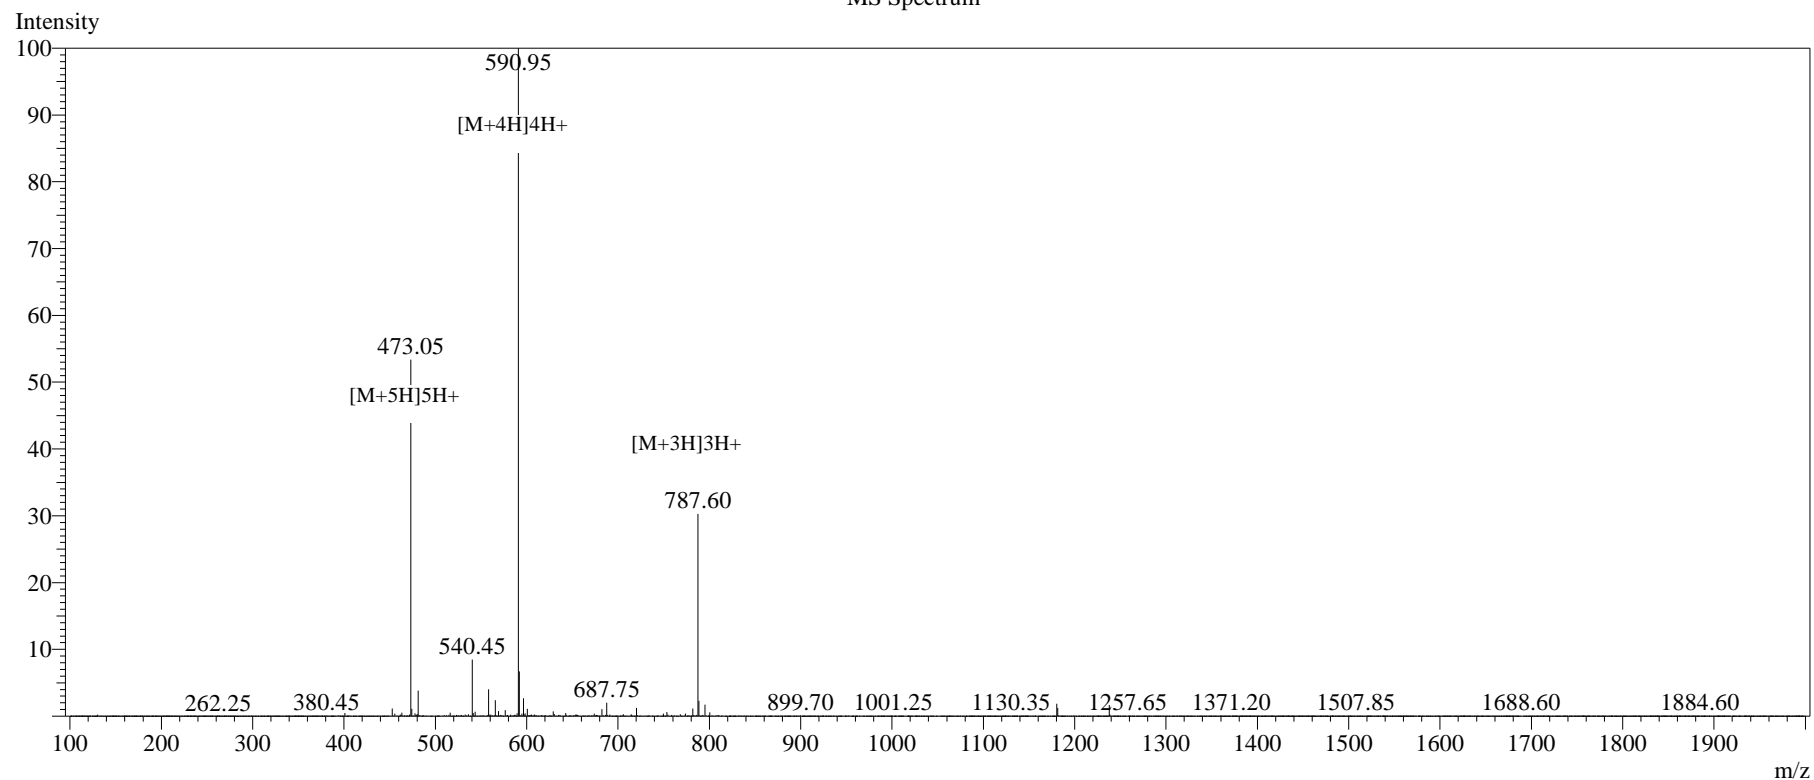

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/06/16 11:43:09	Nebulizing Gas Flow	:1.50L/min	Detector	: -0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% ME OH

Order ID	:MTFA32941
Name	:LANA peptide
Sequence	:MAPPGMRLRSGRSTGAPLTRGSC
Lot.No	:MTFA32941-250613
Theoretical	:2359.73
Observed	:2359.80