

CERTIFICATE OF ANALYSIS

Product Name	P60 peptide, Cat.#: 319340
Lot No.	MTFA31306-0426
Sequence	RDFQSFRKMWPFFAM
Dissolution condition	100%H2O
Length	15AA
Modification	N/A
Molecular Weight (MW)	1994.34
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1994.55	Conforms
Purity by HPLC	>95%	99.083%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Apr/30/2024




Sample Information

Order ID :MTFA31306
 Name :P60
 Sequence :RDFQSFRKMWPFFAM
 Lot. No :MTFA31306-0426
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Phenomenex Luna® 5 µm C18(2) (4.6*250mm*5 µm)
 Dissolution method :100%H2O
 Inj. Volume : 18ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	25
25.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	25
50.00	Controller	Stop	

Chromatogram

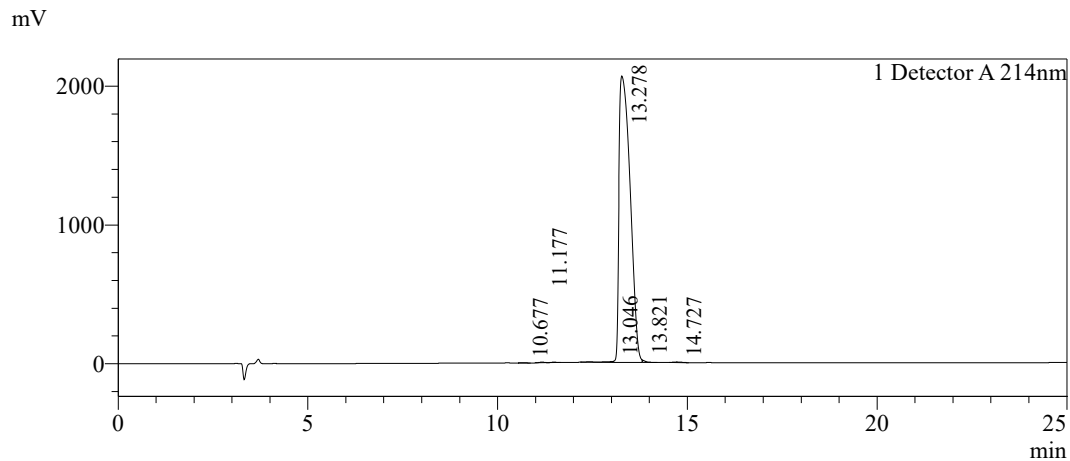


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.677	23544	2590	0.055
2	11.177	80601	4590	0.189
3	13.046	138151	6991	0.324
4	13.278	42211017	2063264	99.083
5	13.821	89294	16108	0.210
6	14.727	59087	4023	0.139
Total		42601695	2097566	100.000

MS Spectrum

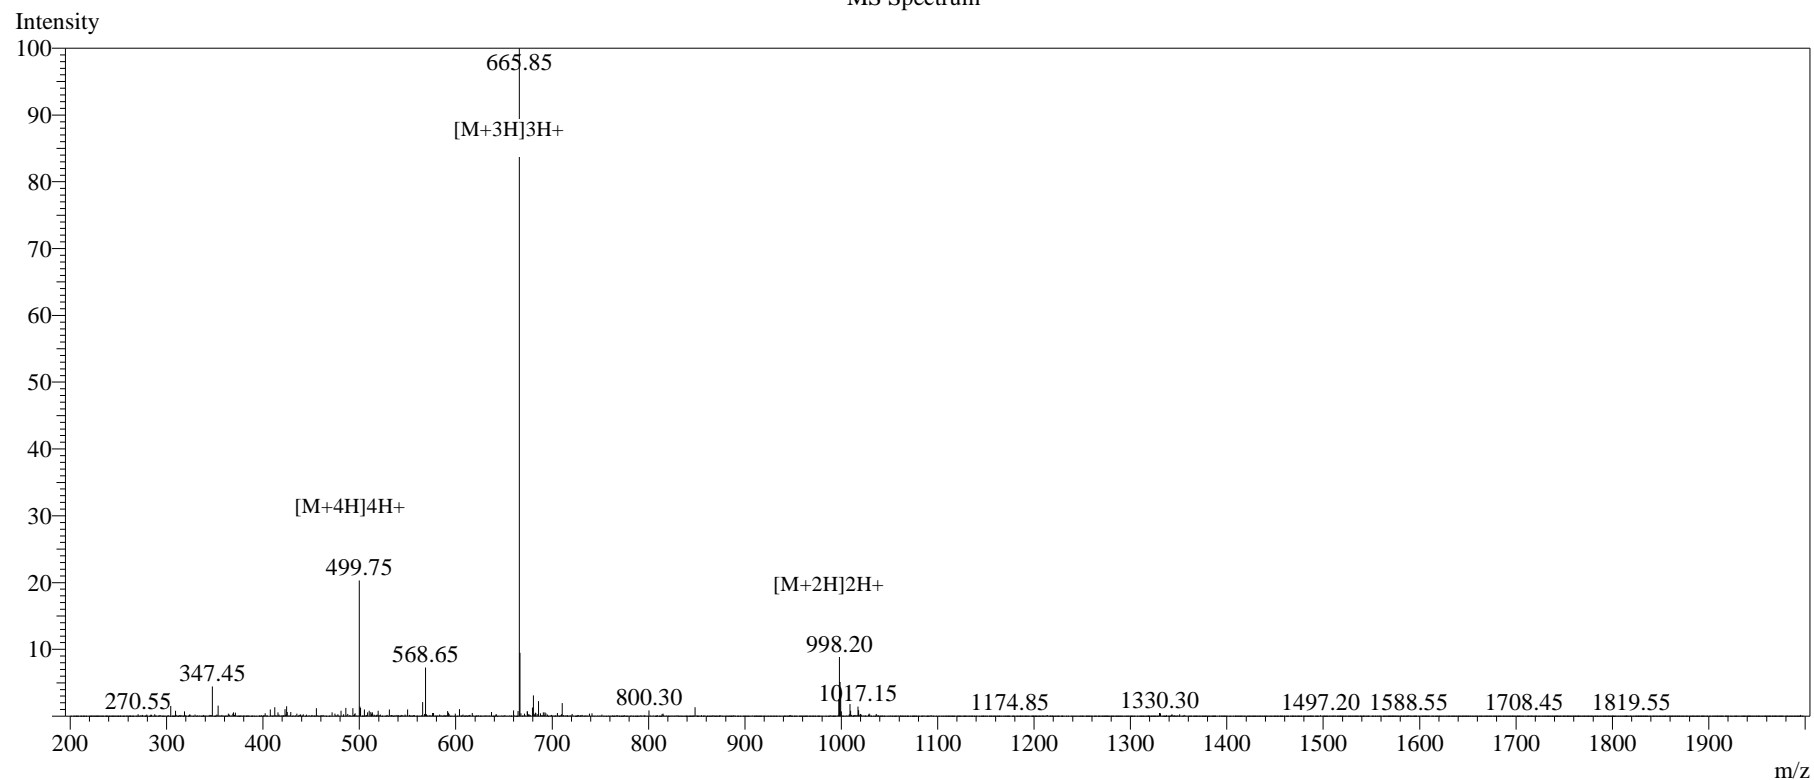

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/04/29 10:22:47	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA31306
Name	:P60
Sequence	:RDFQSFRKMWPFFAM
Lot.No	:MTFA31306-0426
Theoretical	:1994.34
Observed	:1994.55