


CERTIFICATE OF ANALYSIS

Product Name	RVG29 peptide, Cat.#: 319149
Lot No.	MTFA32294-0106
Sequence	YTIWMPENPRPGTPCDIFTNSRGKRASNG
Dissolution condition	100%H ₂ O
Length	29AA
Modification	N/A
Molecular Weight (MW)	3266.63
Storage	-20°C

Test Items	Specifications	Results
MW by MS	3267.25	Conforms
Purity by HPLC	>95%	95.251%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	50mg	5.0mg*10

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department


Jan/08/2025



Sample Information

Order ID	:MTFA32294		
Name	:RVG29 peptide		
Sequence	:YTIWMPENPRPGTPCDIFTNSRGKRASNG		
Lot. No	:MTFA32294-0106		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 μm)		
Dissolution method	:100%H2O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

Chromatogram

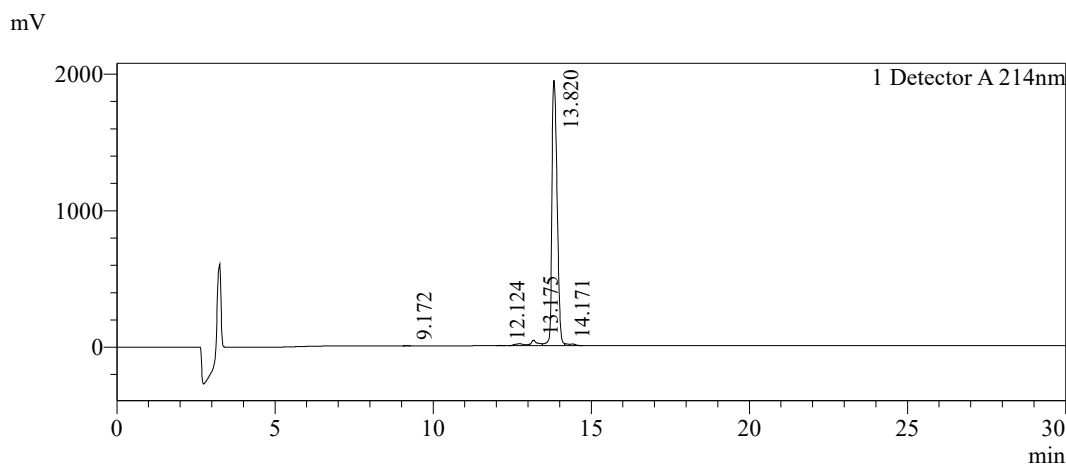


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	9.172	11633	1729	0.050
2	12.124	14900	1665	0.063
3	13.175	843639	39933	3.594
4	13.820	22357152	1942843	95.251
5	14.171	244542	14096	1.042
Total		23471867	2000266	100.000

MS Spectrum

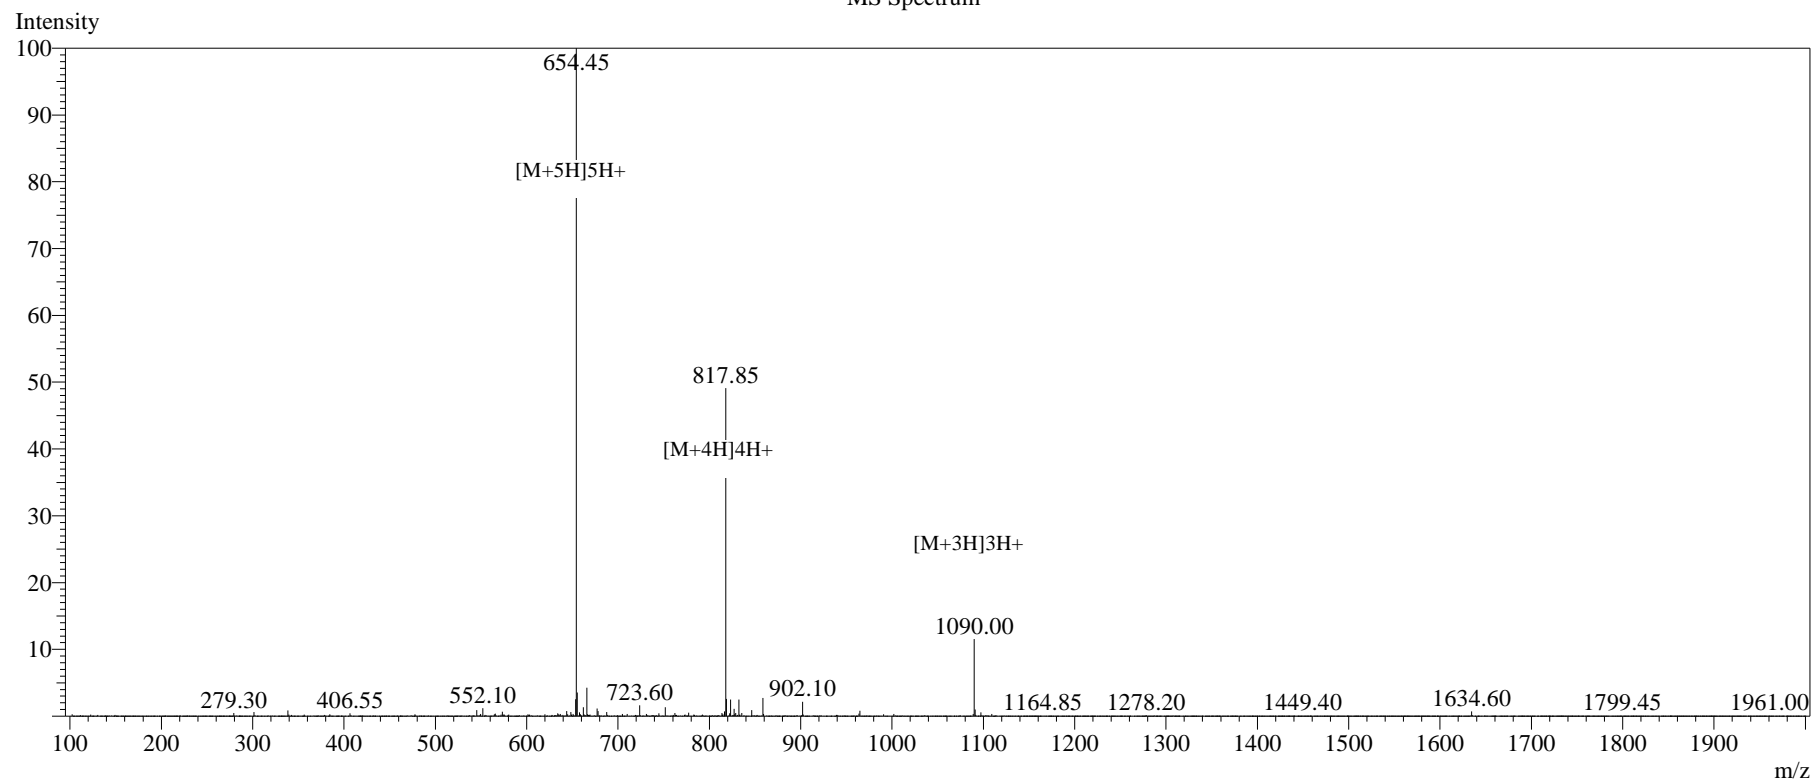

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/01/07 10:18:15	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H2O/50% MEOH
Order ID	:MTFA32294				
Name	:RVG29 peptide				
Sequence	:YTIWMPENPRPGTPCDIFTNSRGKRASNG				
Lot.No	:MTFA32294-0106				
Theoretical	:3266.63				
Observed	:3267.25				